


# **Stretchable wireless sensor could monitor healing of cerebral aneurysms**

August 28 2019

---

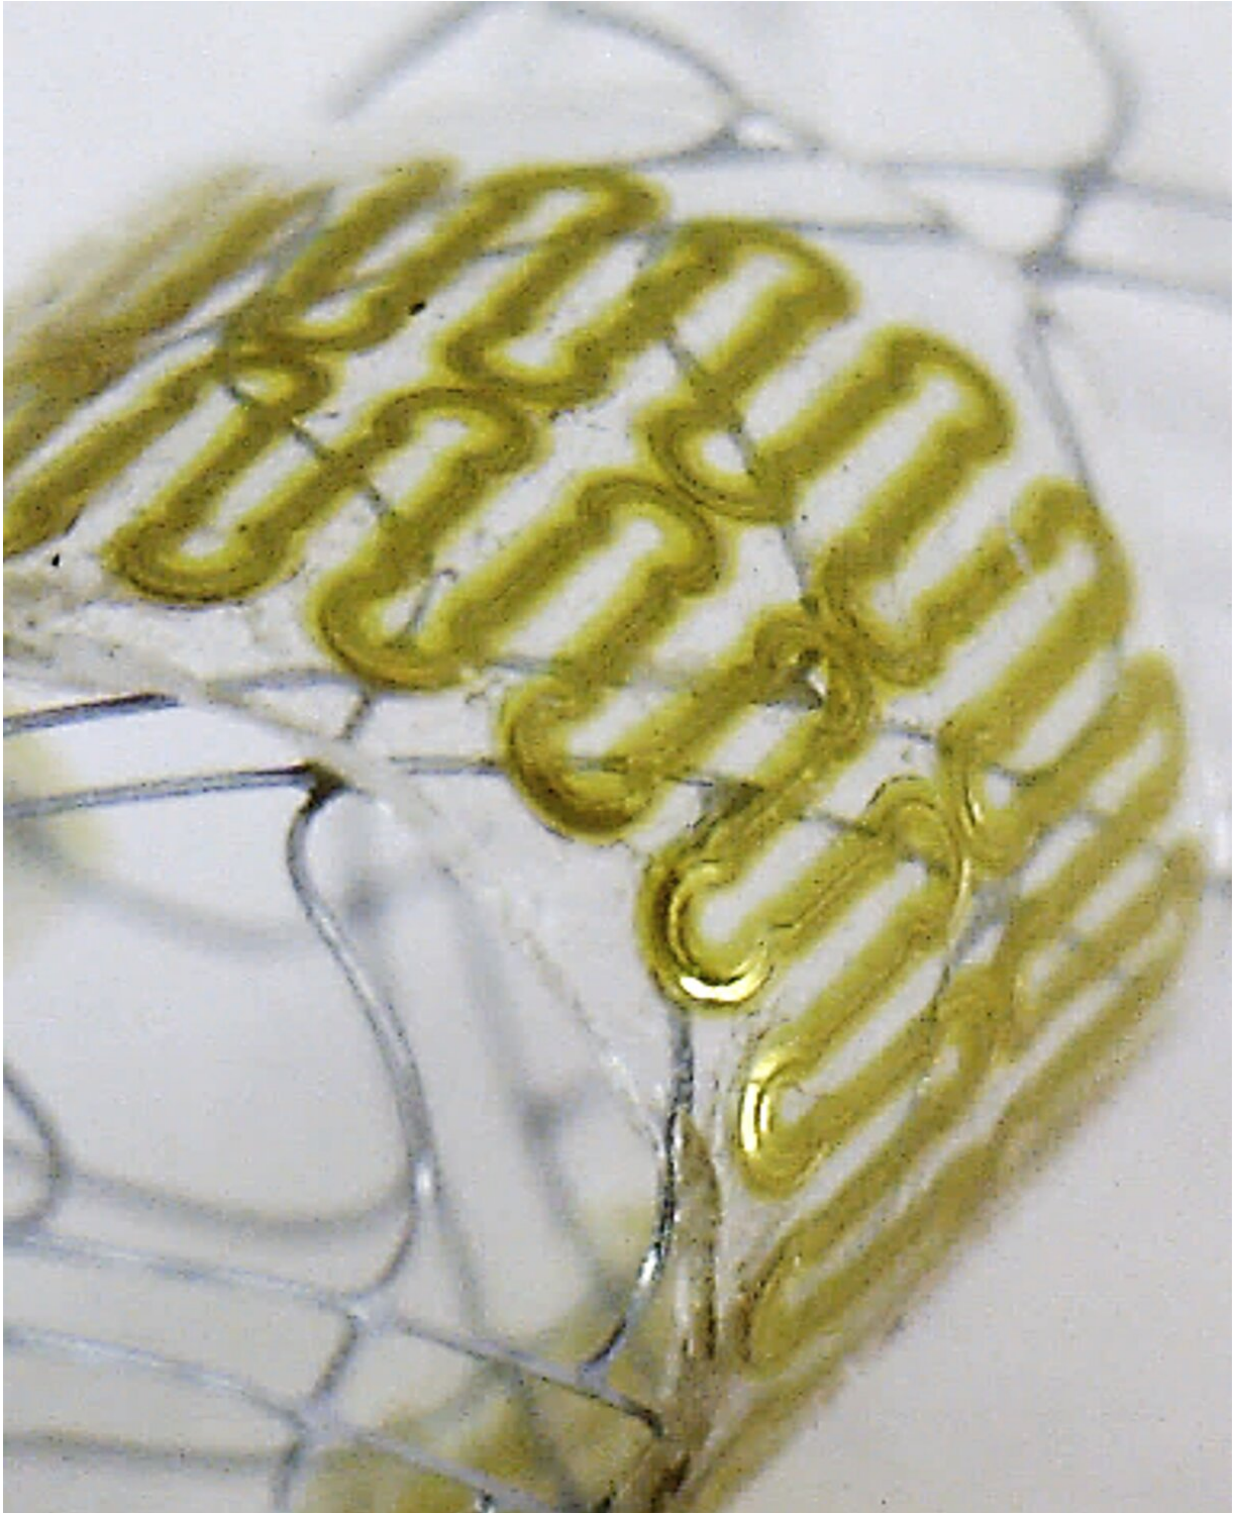

This close-up image shows details of the ultra-thin, low-profile sensor for monitoring blood flow in the brain. Credit: Georgia Tech

A wireless sensor small enough to be implanted in the blood vessels of the human brain could help clinicians evaluate the healing of aneurysms—bulges that can cause death or serious injury if they burst. The stretchable sensor, which operates without batteries, would be wrapped around stents or diverters implanted to control blood flow in vessels affected by the aneurysms.


To reduce costs and accelerate manufacturing, fabrication of the stretchable [sensors](#) uses aerosol jet 3-D printing to create conductive silver traces on elastomeric substrates. The 3-D additive manufacturing technique allows production of very small electronic features in a single step, without using traditional multi-step lithography processes in a cleanroom. The device is believed to be the first demonstration of aerosol jet 3-D printing to produce an implantable, stretchable sensing system for wireless monitoring.

"The beauty of our sensor is that it can be seamlessly integrated onto existing medical stents or flow diverters that clinicians are already using to treat aneurysms," said Woon-Hong Yeo, an assistant professor in Georgia Tech's George W. Woodruff School of Mechanical Engineering and the Wallace H. Coulter Department of Biomedical Engineering at Georgia Tech and Emory University. "We could use it to measure an incoming blood flow to the [aneurysm](#) sac to determine how well the aneurysm is healing, and to alert doctors if blood flow changes."

Inserted using a catheter system, the sensor would use inductive coupling of signals to allow wireless detection of biomimetic cerebral aneurysm hemodynamics. The research was reported August 7 in the journal *Advanced Science*.

Monitoring the progress of cerebral aneurysms now requires repeated

angiogram imaging using contrast materials that can have harmful side effects. Because of the cost and potential negative effects, use of the imaging technique must be limited. However, a sensor placed in a blood vessel could allow more frequent evaluations without the use of imaging dyes.

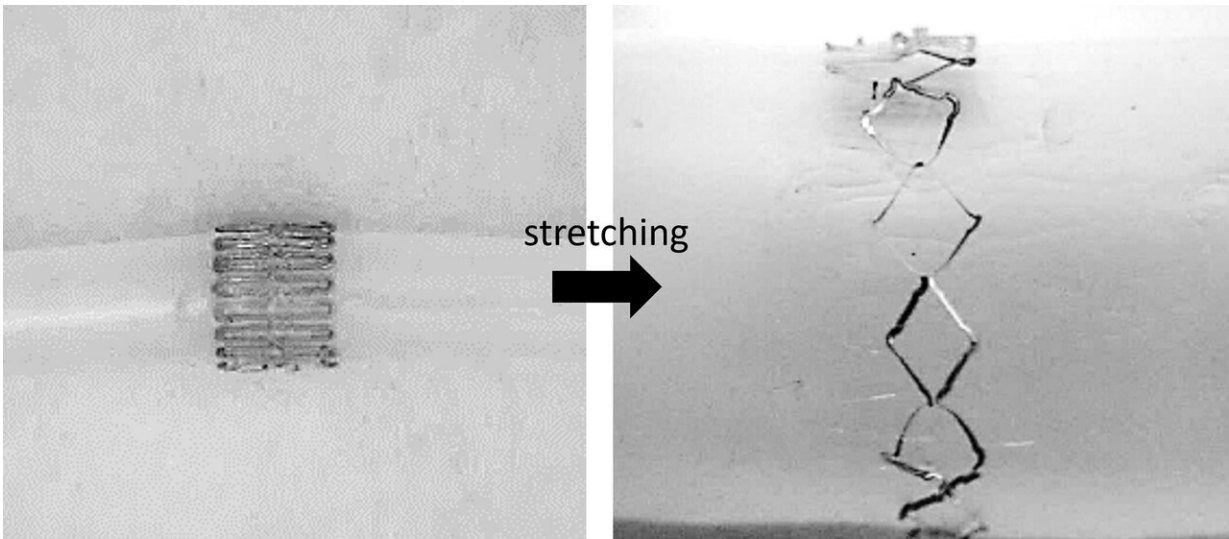

The wireless blood flow sensor is stretchable, allowing it to conform to a stent for implantation. Credit: Georgia Tech

"For patients who have had a procedure done, we would be able to tell if the aneurysm is occluding as it should without using any imaging tools," Yeo said. "We will be able to accurately measure blood flow to detect changes as small as 0.05 meters per second."

The six-layer sensor is fabricated from biocompatible polyimide, two separate layers of a mesh pattern produced from silver nanoparticles, a dielectric and soft polymer-encapsulating material. The sensor would be wrapped around the stent or flow diverter, which must be less than two




or three millimeters in diameter to fit into the [blood](#) vessels.

The sensor includes a coil to pick up electromagnetic energy transmitted from another coil located outside the body. Blood flowing through the implanted sensor changes its capacitance, which alters the signals passing through the sensor on their way to a third coil located outside the body. In the laboratory, Yeo and his collaborators have measured capacitance changes six centimeters away from a sensor implanted in meat to simulate brain tissue.

"The flow rate is correlated really well with the capacitance change that we can measure," Yeo said. "We have made the sensor very thin and deformable so it can respond to small changes in [blood flow](#)."

Use of the aerosol jet 3-D printing technique was essential to producing the stretchable and flexible electronics necessary for the sensor. The technique uses a spray of aerosol particles to create patterns, allowing narrower feature sizes than conventional inkjet printing.

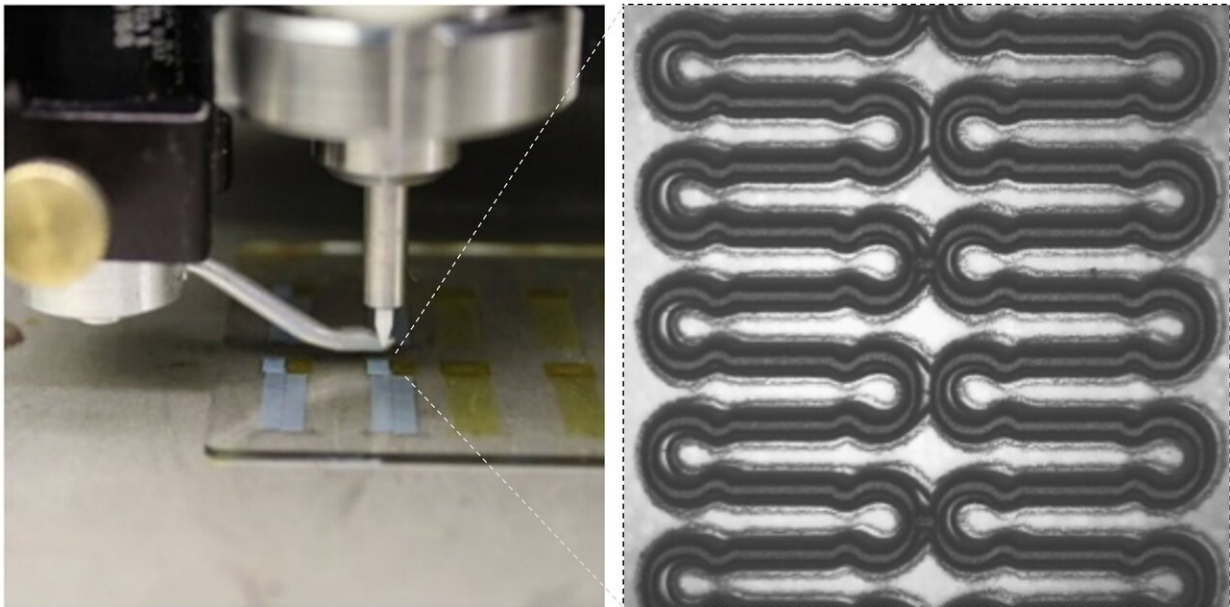

The wireless sensors are produced using an aerosol jet 3D printer. An example of the silver nanoparticle film is shown on the right. Credit: Georgia Tech

"We can control the printing speed, the printing width, and the amount of material being jetted," Yeo said. "The parameters can be optimized for each material, and we can use materials that have a broad range of viscosities."

Because the sensor can be fabricated in a single step without costly cleanroom facilities, it could be manufactured in higher volume at lower cost.

The next phase of the aneurysm sensor will be able to measure [blood pressure](#) in the vessel along with the flow rates. "We will be able to measure how pressure contributes to flow change," Yeo explained. "That would allow the device to be used for other applications, such as intracranial pressure measurements."

Yeo's research team has also developed a flexible and wearable health monitor able to provide ECG and other information. He says the success of the monitoring technique demonstrates the potential for smart and connected wireless soft electronics based on nanomaterials, stretchable mechanics, and machine learning algorithms.

"We are excited that people are now recognizing the potential of this technology," Yeo added. "There are a lot of opportunities to integrate this sensing mechanism into ultrathin membranes that are implantable within the body."

**More information:** Robert Herbert et al, Fully Printed, Wireless,

Stretchable Implantable Biosystem toward Batteryless, Real-Time Monitoring of Cerebral Aneurysm Hemodynamics, *Advanced Science* (2019). [DOI: 10.1002/advs.201901034](https://doi.org/10.1002/advs.201901034)

Provided by Georgia Institute of Technology

Citation: Stretchable wireless sensor could monitor healing of cerebral aneurysms (2019, August 28) retrieved 20 March 2024 from <https://techxplore.com/news/2019-08-stretchable-wireless-sensor-cerebral-aneurysms.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.