

World's thinnest, lightest signal amplifier enables bioinstrumentation with reduced noise

August 20 2019

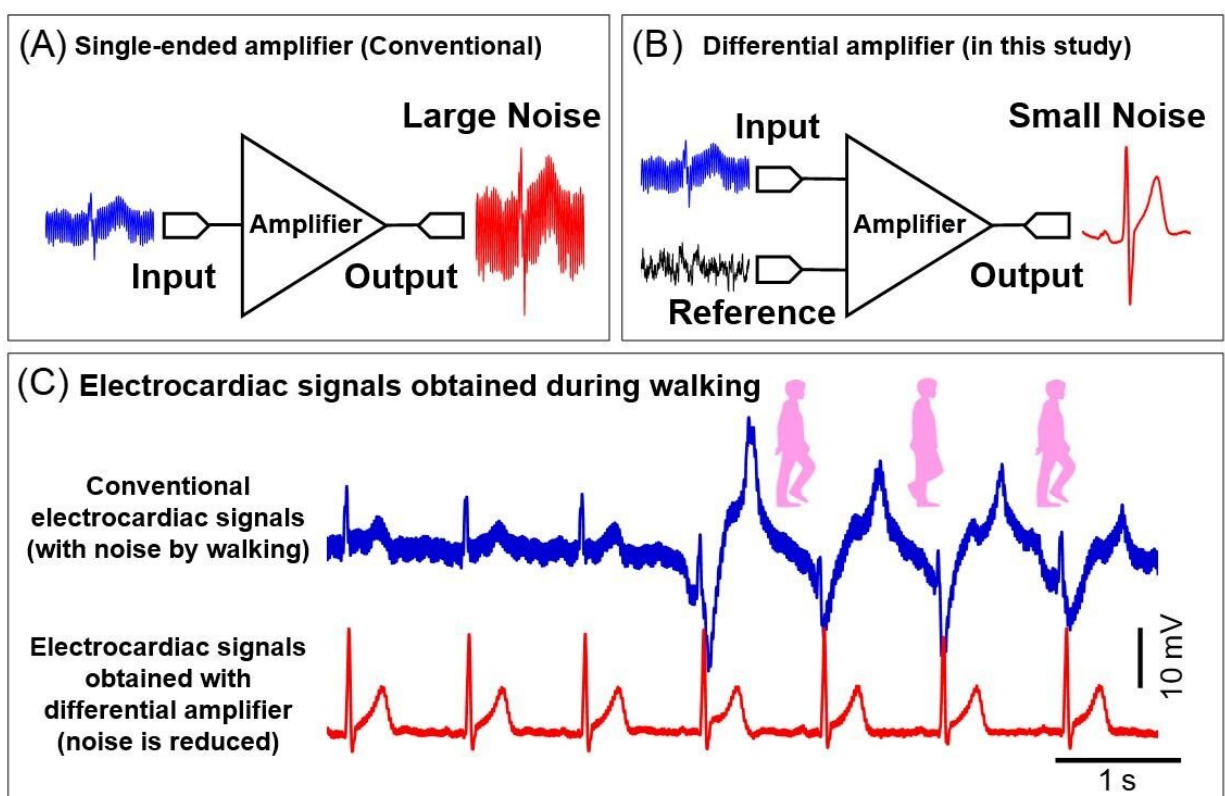


Fig. 1. Electrocardiac signals obtained using flexible organic differential amplifier (A)Conventional single-ended amplifier(B)Differential amplifier developed in this study(C)Electrocardiac signals obtained from a walking subject. In the electrocardiac signals obtained using a conventional single-ended amplifier, large noise caused by walking is included in the waveform. In contrast, such noise is removed from the waveform obtained using the developed flexible organic differential amplifier. Credit: Osaka University

A research group led by Professor Tsuyoshi Sekitani and Associate Professor Takafumi Uemura of The Institute of Scientific and Industrial Research, Osaka University, succeeded in developing the world's thinnest and lightest differential amplifier for bioinstrumentation.

Conventionally, bioinstrumentation circuits for health care and medical use have consisted of hard electronic devices, such as silicon transistors. However, when soft biological tissues, such as skin, come into contact with hard electronic devices, they tend to become inflamed. Therefore, monitoring of biosignals in [everyday life](#) over a long period of time proved difficult. The research group developed a flexible bioinstrumentation circuit that eliminates the discomfort caused by the device attached to the body of the user by integrating flexible electronic devices called [organic transistors](#) on a thin and flexible plastic film with a thickness of 1 μm . The developed circuit is a signal-processing circuit called a differential [amplifier](#).

Compared with conventional single-ended amplifiers, the flexible differential amplifier developed in this study can not only amplify very weak biopotential but also reduce disturbance [noise](#). This group demonstrated that the differential amplifier can be applied to human instrumentation and realize real-time monitoring of electrocardiac signals, which are important biosignals, with reduced noise levels.

This achievement is expected to lead to the monitoring of various weak biosignals (e.g. brain waves and cardiac sounds of a fetus) in everyday life in addition to electrocardiac signals without subjecting users to the discomfort caused by devices attached to the body.

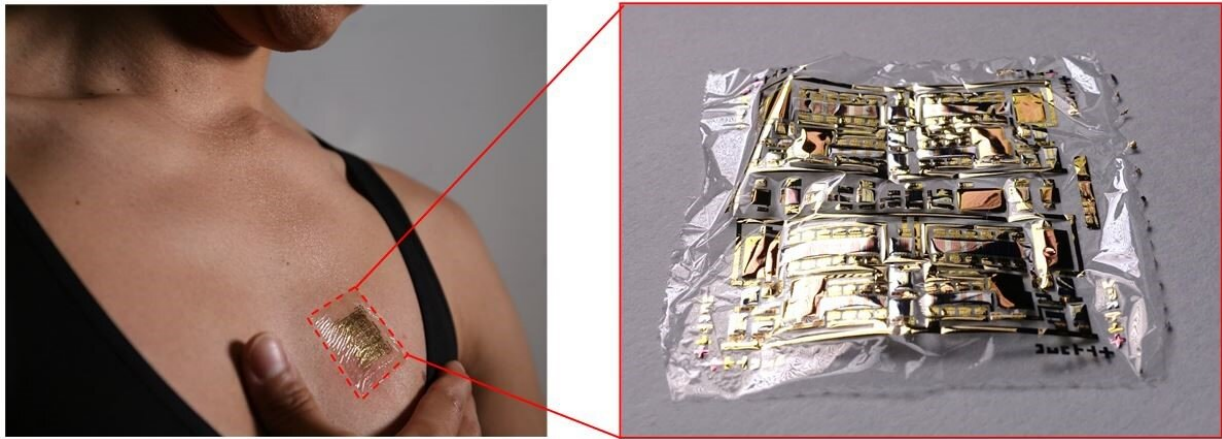


Fig. 2. Flexible organic differential amplifier attached onto the human chest The organic differential amplifier is extremely lightweight and thin and can be attached onto soft skin without causing any discomfort to the user. Bioinstrumentation in everyday life is expected to become simpler and more comfortable to use. Credit: Osaka University

In Japan, with its declining birthrate and aging population, the application of flexible electronics such as organic transistors in the medical and health care fields has been actively promoted. Sensors and electronic circuits with a high compatibility with biological tissues such as skin and organs are realized by using soft organic materials.

Among these sensors and electronic circuits, flexible amplifiers with organic transistors integrated into them eliminate the discomfort felt by users caused by the devices attached to the body. The research and development of such amplifiers as sensors to continuously monitor very weak biosignals is currently ongoing. However, conventional organic amplifiers mainly have a single-ended structure that cannot distinguish the target biosignals from disturbance noise, making it difficult to monitor biosignals with a low noise level (Fig. 1). A differential amplifier is a circuit that can measure signals with the noise components

removed. However, the variation in the quality of manufactured organic transistors is large compared with that of [silicon transistors](#); thus, there have been no reports on flexible differential amplifiers that realize precise noise reduction.

The research group succeeded in developing a flexible organic differential amplifier with a noise reduction function by developing a compensation technique that can reduce the dispersion of current flowing in organic [transistors](#) inside the amplifier to as small as 2% or less. The amplifier was fabricated on a parylene film with a thickness of 1 μm . The amplifier does not break when the film is bent and can be attached to human skin without causing any discomfort (Fig. 2).

Electrocardiac signals were amplified 25-fold and the noise was reduced to one-seventh or less by using this flexible differential amplifier for monitoring the signals. The group demonstrated that the noise caused by external power sources as well as large body-motion noise caused by walking are removed during the monitoring of electrocardiac signals (Fig. 1).

Smart watches and other wearable devices for monitoring biosignals, such as electrocardiac signals, in everyday life are already on the market. Bioinstrumentation is expected to become easier and more comfortable in various situations through the use of the high-precision flexible bioinstrumentation [circuits](#) without subjecting users to any discomfort caused by the devices attached to their body. For example, bioinstrumentation of people who are performing physically strenuous exercise, such as during sports, becomes possible owing to the improved wearability and adhesion between the [device](#) and skin. The real-time long-time bioinstrumentation data thus obtained will promote early detection of diseases and improve the efficiency of treatment, monitoring of the elderly and patients, and [monitoring](#) of exercise load. These achievements will further lead to the solution of various problems in Japan's aging society by way of reduced medical expenses and

improved quality of life (QOL).

The article, "An ultraflexible organic differential amplifier for recording electrocardiograms" was published in *Nature Electronics*.

More information: Masahiro Sugiyama et al. An ultraflexible organic differential amplifier for recording electrocardiograms, *Nature Electronics* (2019). [DOI: 10.1038/s41928-019-0283-5](https://doi.org/10.1038/s41928-019-0283-5)

Provided by Osaka University

Citation: World's thinnest, lightest signal amplifier enables bioinstrumentation with reduced noise (2019, August 20) retrieved 6 May 2024 from <https://techxplore.com/news/2019-08-world-thinnest-lightest-amplifier-enables.html>

<p>This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.</p>
--