


# Liquid metal may point way to wearable ultrasound devices

March 20 2024, by Scott Schrage

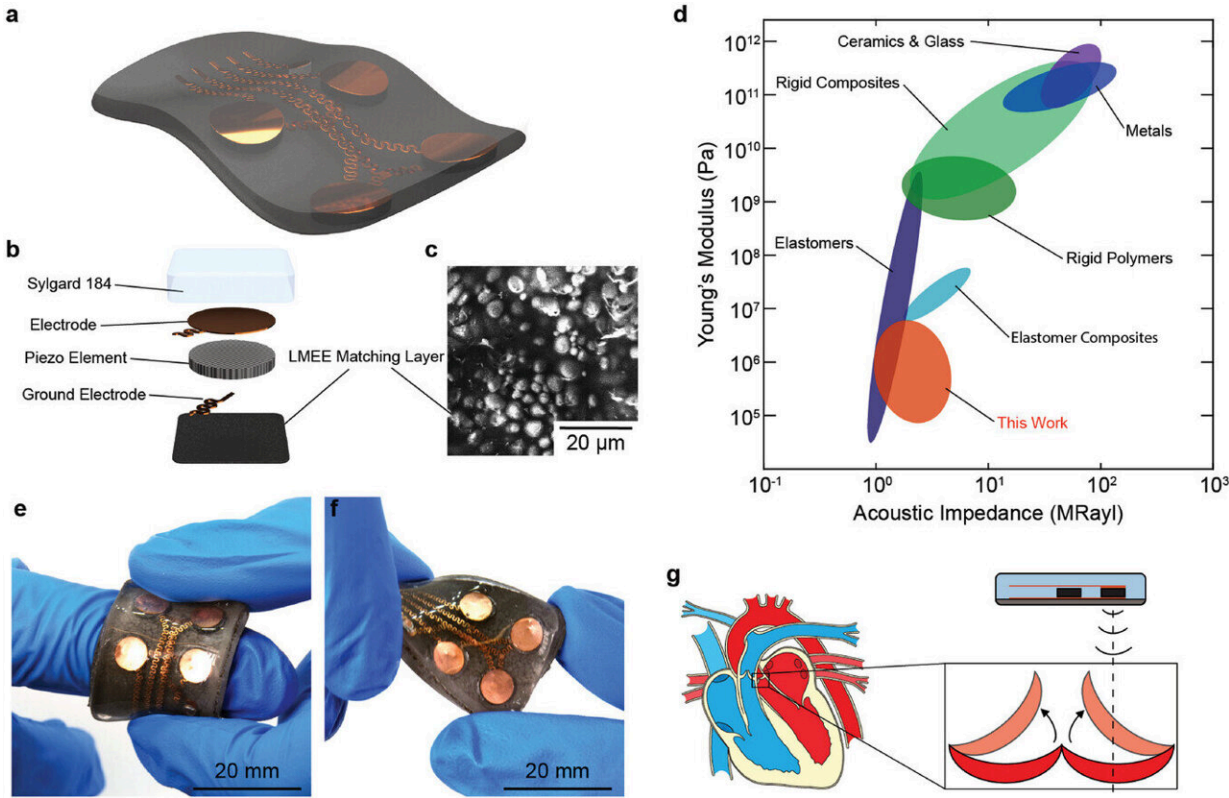

LM-elastomer composites with tunable acoustic impedance. a) Schematic illustration and b) exploded view illustration of a stretchable ultrasonic transducer array with LM-elastomer composite matching layer. c) SEM micrograph of LM droplets embedded in elastomer matrix. d) Plot of Young's modulus versus acoustic impedance for various impedance matching layers. e,f) Photographs of the stretchable ultrasound device with LM-elastomer composite matching layer under deformation. g) Schematic illustration of possible application of the stretchable ultrasound array with matching layer where heart

valve motion is continuously monitored. Credit: *Advanced Functional Materials* (2023). DOI: 10.1002/adfm.202308954

The best-known byproduct of ultrasound—so named because its frequencies exceed the range of the human ear—is, in fact, not audio but visual: 2D imagery, often of a fetus maturing in the womb. But ultrasound has also found a place in other corners of the medical realm, from assessing blood flow to examining suspicious lumps and diagnosing disease.

That diagnostic capability has recently motivated [biomedical engineers](#) to design wearable [ultrasound](#) devices that can continuously monitor for signs of trouble, particularly by tracking [blood flow](#) or the rhythmic motion of the heart. Those [wearable devices](#) will ideally consist of stretchable material that accommodates movement and the human form.

Unfortunately, a stubborn engineering challenge stands in the way. Ultrasound relies on transducers, which both emit the high-frequency sound waves and detect those reflected back by various structures in the body, ultimately forming an image. Reflections occur wherever the waves cross a boundary between two materials that offer different levels of resistance, or acoustic impedance.

To overcome the differing acoustic impedance that waves face in passing from a transducer to the human body—a mismatch that ruins acoustic transmission—engineers install so-called matching layers between the two. Most particles or materials employed as matching layers, though, have proven too rigid for use in pliable, wearable devices.

Nebraska's Eric Markvicka, Ethan Krings and colleagues have spent years investigating the properties and potential applications of liquid

metal droplets, which include gallium-based alloys. With an eye toward designing a more conforming but still-functional matching layer, the Husker researchers embedded various volumes and sizes of gallium-based droplets in a soft silicone.

When saturating the silicone with roughly 70% of the droplets, the team found that the resulting density of the matching layer increased its acoustic impedance by more than 400%—to levels approaching those boasted by more rigid counterparts. And that impedance declined by only 13% when the matching layer was mechanically strained in ways akin to what it might endure as part of a wearable device.

The team then collaborated with Nebraska's Greg Bashford and Ben Hage to integrate its stretchable matching layer into a wearable ultrasound prototype. When presented with a moving object that simulated the motion of a heart valve or other tissue, the prototype successfully registered that movement, demonstrating its potential as a diagnostic device.

Their findings are [published](#) in the journal *Advanced Functional Materials*.

Modifying the liquid metal droplets, whether by tailoring their surfaces or their alloys, could further improve the performance of the matching layers that incorporate them, the team said. As the [medical field](#) moves toward wearable devices, the researchers said, those matching layers could find their way into specialized ultrasonic sensors that help detect multiple diseases and conditions.

**More information:** Ethan J. Krings et al, Acoustic Properties of Stretchable Liquid Metal-Elastomer Composites for Matching Layers in

Wearable Ultrasonic Transducer Arrays, *Advanced Functional Materials* (2023). [DOI: 10.1002/adfm.202308954](https://doi.org/10.1002/adfm.202308954)

Provided by University of Nebraska-Lincoln

Citation: Liquid metal may point way to wearable ultrasound devices (2024, March 20) retrieved 27 April 2024 from

<https://techxplore.com/news/2024-03-liquid-metal-wearable-ultrasound-devices.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.