


# Brain signal measurement using printed tattoo electrodes

13 May 2020

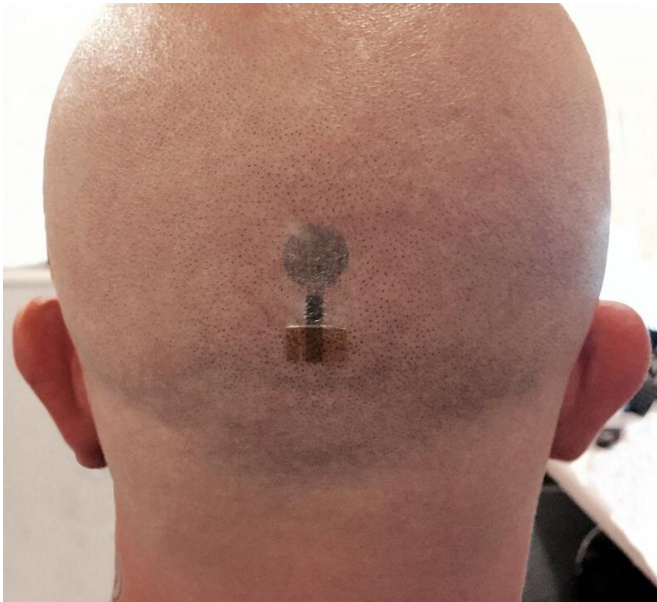

The reliability and accuracy of tattoo electrodes has been successfully tested under real clinical conditions. Credit: Francesco Greco

In 2015 Francesco Greco, head of the Laboratory of Applied Materials for Printed and Soft electronics (LAMPSe) at the Institute of Solid State Physics at Graz University of Technology, developed so-called "tattoo electrodes" together with Italian scientists.

These are conductive polymers that are printed using an [inkjet printer](#) on standard tattoo paper and then stuck to the skin like transfers to measure heart or muscle activity.

This type of [electrode](#), optimized in 2018, opened up completely new paths in electrophysiological examinations, such as electrocardiography (ECG) or electromyography (EMG). Thanks to a thickness of 700 to 800 nanometers—that is about 100 times thinner than a [human hair](#)—the tattoos adapt to


uneven skin and are hardly noticeable on the body.

Moreover, the "tattoos" are dry electrodes; in contrast to gel electrodes, they work without a liquid interface and cannot dry out.

They are excellently suited for long-term measurements. Even hairs growing through the tattoo do not interfere with the signal recording.

## New generation of tattoo electrodes

Building on this pioneering achievement, Greco, together with Esmā Ismailova (Department of Bioelectronics, École Nationale Supérieure des Mines de Saint-Étienne, France) and Laura Ferrari (The BioRobotics Institute, Scuola Superiore Sant'Anna, Italy), has now achieved a further milestone in the measurement of bioelectrical signals: the group has modified the tattoo electrodes in such a way that they can also be used in electroencephalography (EEG) – i.e. to measure brain activity.

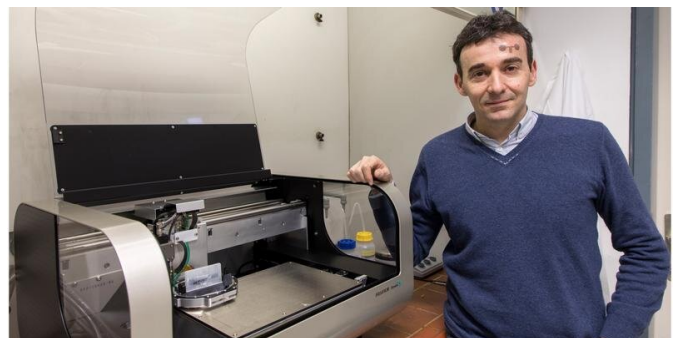

Francesco Greco and his team at the Institute of Solid State Physics at TU Graz are developing electrodes in the form of temporary tattoos for the long-term monitoring of bioelectric signals. Credit: Lunghammer

To do this, the researchers used the same

approach as in 2018, i.e. inkjet printing of conductive polymer on tattoo paper. The composition and thickness of the transfer paper and conductive polymer have been optimized to achieve an even better connection between the tattoo electrode and the skin and to record the EEG signals with maximum quality, because:

"Brain waves are in the low frequency range and EEG signals have a very low amplitude. They are much more difficult to capture in high quality than EMG or ECG signals," explains Laura Ferrari, who worked on this project during her Ph.D. and is now a postdoc researcher in France.

Tests under real clinical conditions have shown that the EEG measurement with the optimized tattoos is as successful as with conventional EEG electrodes.

"Due to inkjet printing and the commercially available substrates, however, our tattoos are significantly less expensive than current EEG electrodes and also offer more advantages in terms of wearing comfort and long-term measurements in direct comparison," says Greco.

### First ever MEG-compatible dry electrodes

The new tattoo electrodes are the very first dry electrode type that is suitable for long-term EEG measurements and at the same time compatible with magneto-encephalography (MEG). MEG is a well-established method for monitoring [brain activity](#), for which so far only so-called "wet electrodes" can be used.

Such electrodes work on the basis of electrolyte, gel or an electrode paste, and thus dry out quickly and are unsuitable for long-term measurements. The new generation of [tattoo electrodes](#) consists exclusively of [conductive polymers](#), i.e. it does not contain any metals which can be problematic for MEG examinations, and is printed exclusively with inkjet.

"With our method, we produce the perfect MEG-compatible electrode while reducing costs and production time," says Greco happily. The TU Graz researcher is currently spinning ideas on how this technology can be used in clinics and in

neuroengineering as well as in the field of brain computer interfaces.

Details of the latest development of the Styrian-Italian-French research alliance can be read in the journal *npj Flexible Electronics*.

**More information:** Laura M. Ferrari et al. Conducting polymer tattoo electrodes in clinical electro- and magneto-encephalography, *npj Flexible Electronics* (2020). [DOI: 10.1038/s41528-020-0067-z](https://doi.org/10.1038/s41528-020-0067-z)

Provided by Graz University of Technology

APA citation: Brain signal measurement using printed tattoo electrodes (2020, May 13) retrieved 4 December 2020 from <https://techxplore.com/news/2020-05-brain-tattoo-electrodes.html>

*This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.*